

1/5

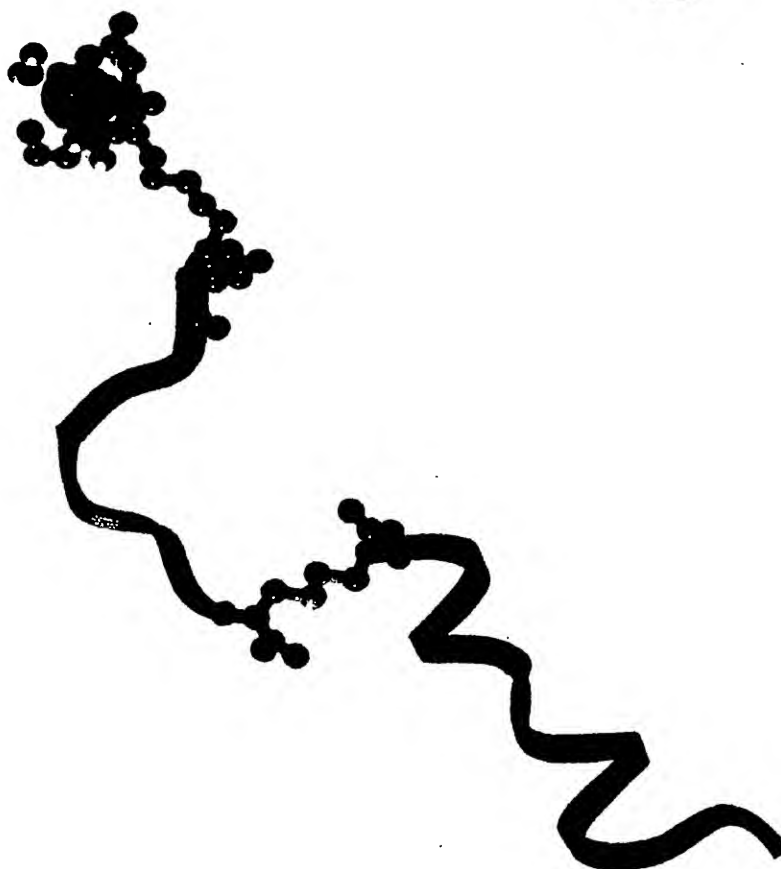
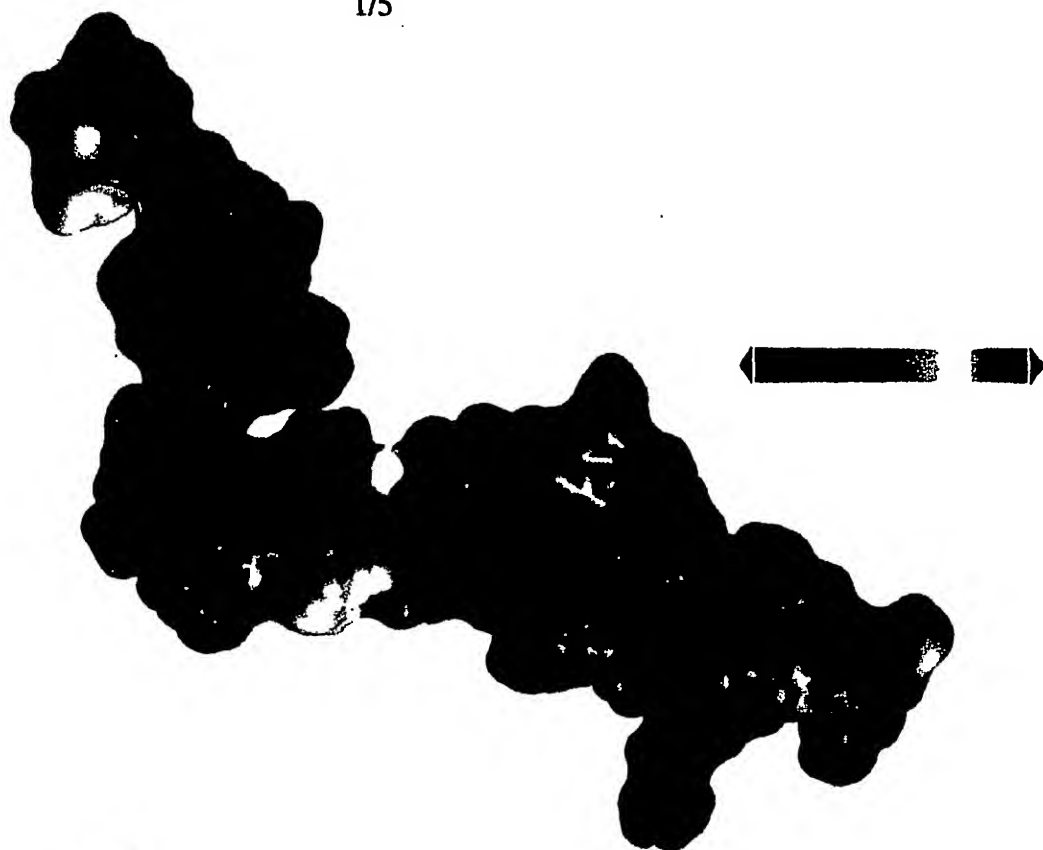


Fig. 1

2/5

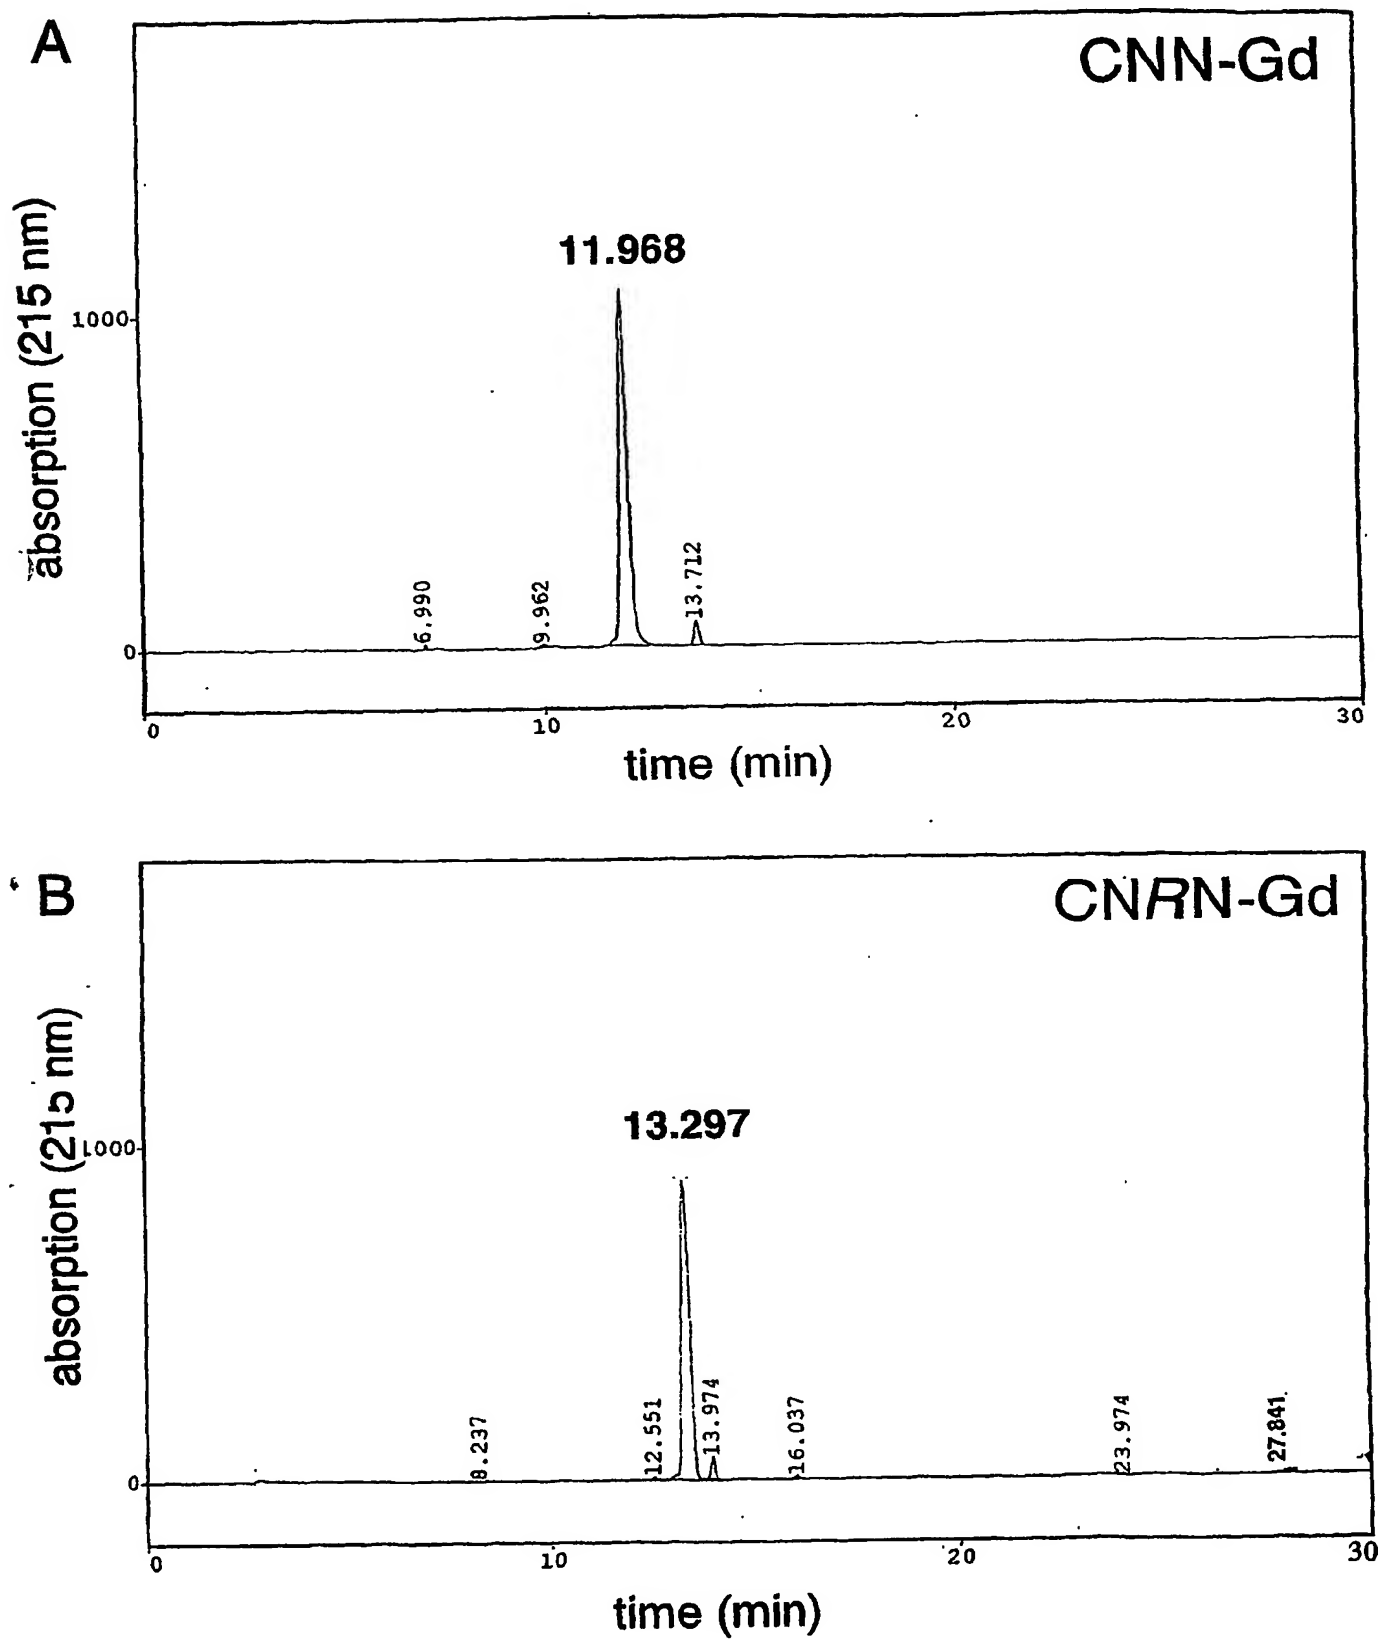


Fig. 2



VISION 2000

Data File: VISIONDATA010698.001

Sample:

C21298

Comment:

Number of shots: 3

Operator:

Positive Ions

Laser Power: 64

External Calibration

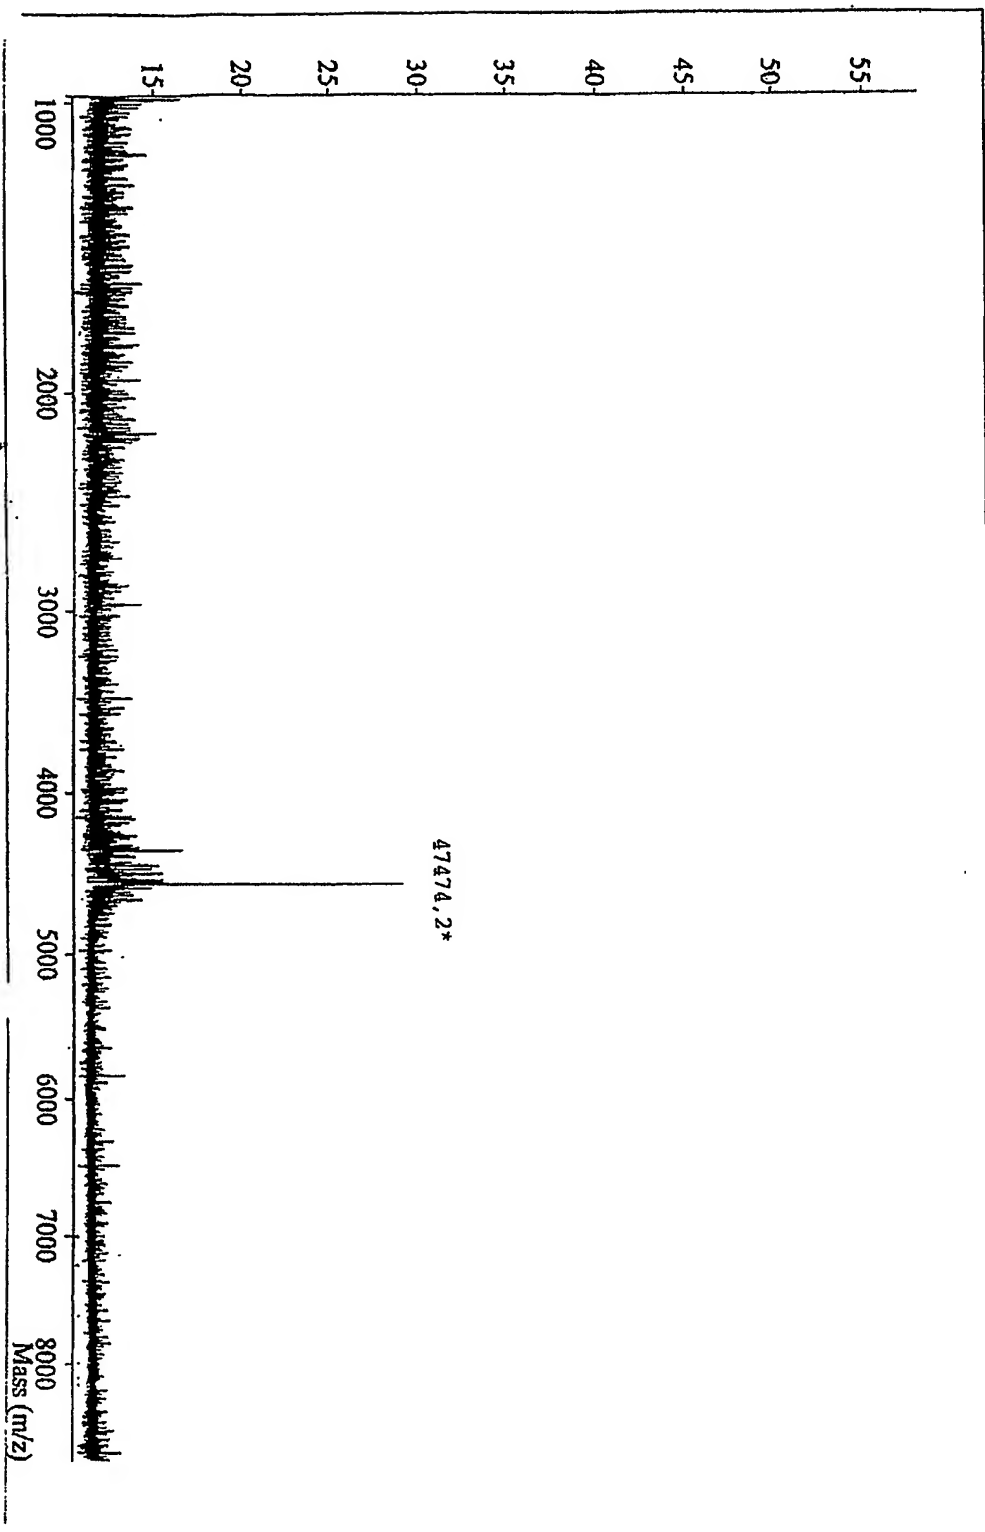


Fig. 3


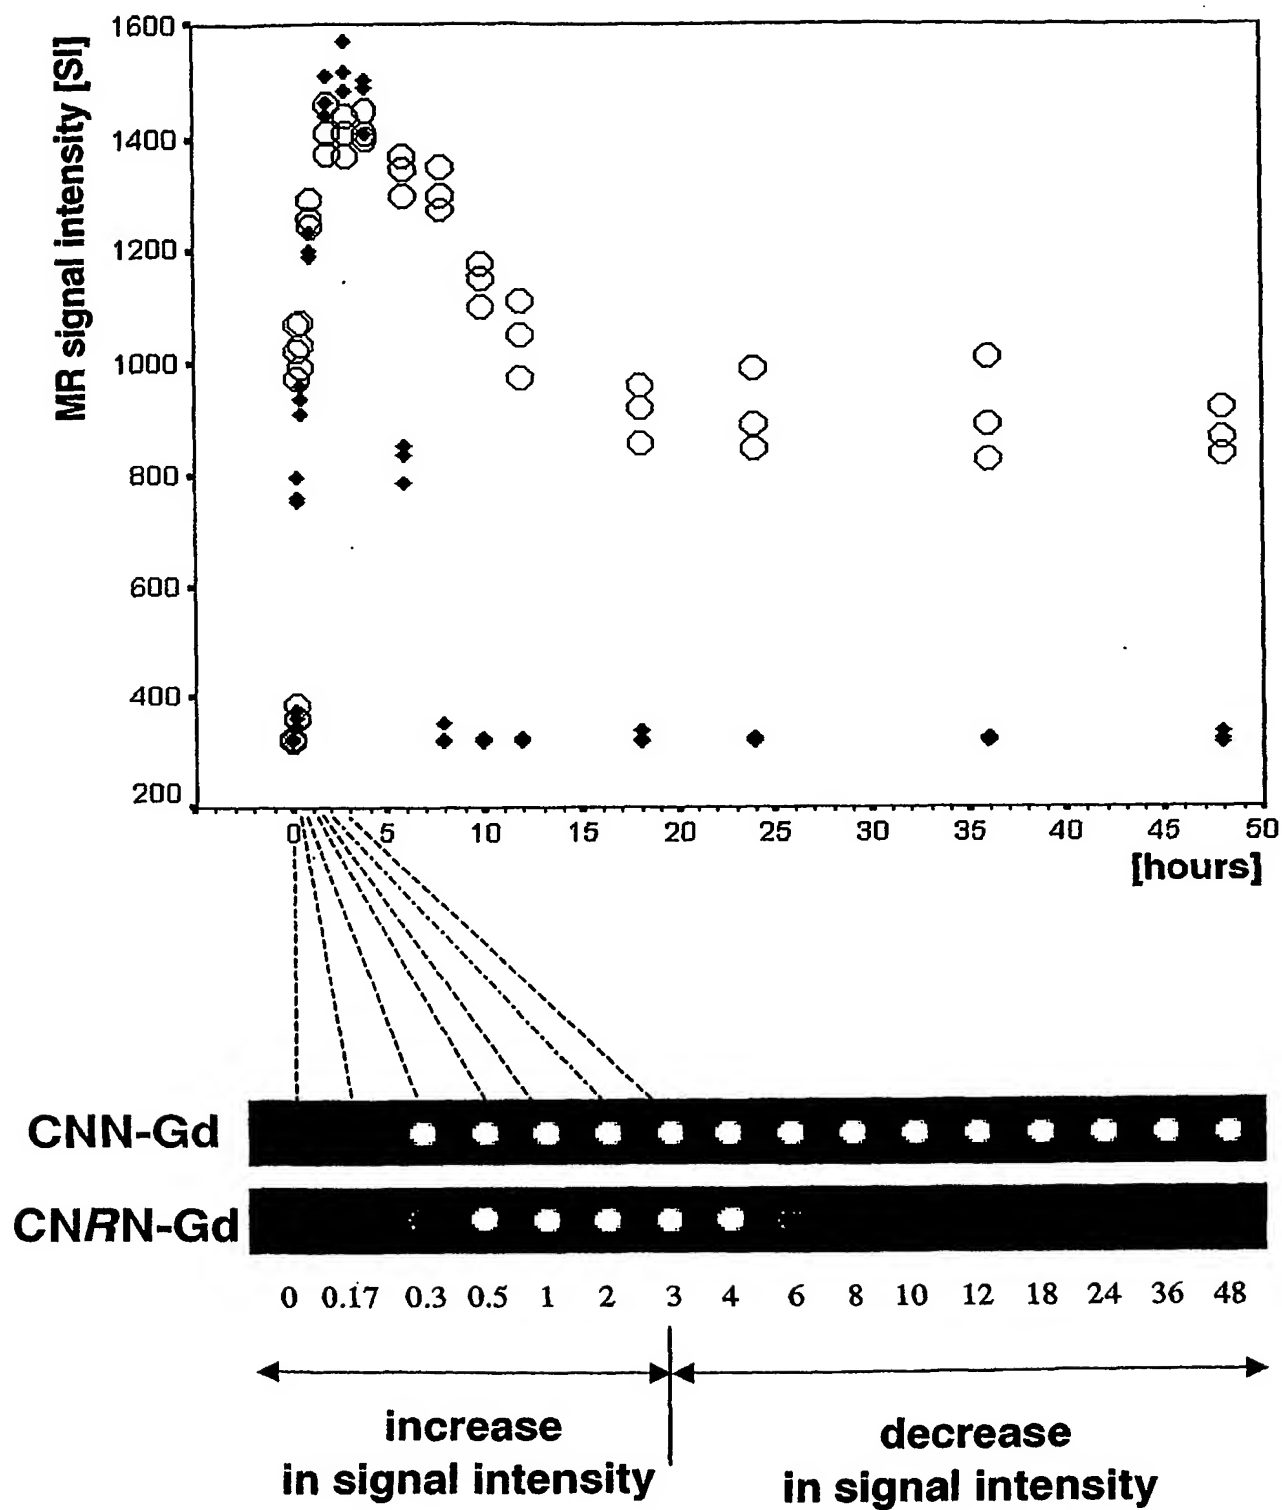


Fig. 4

a

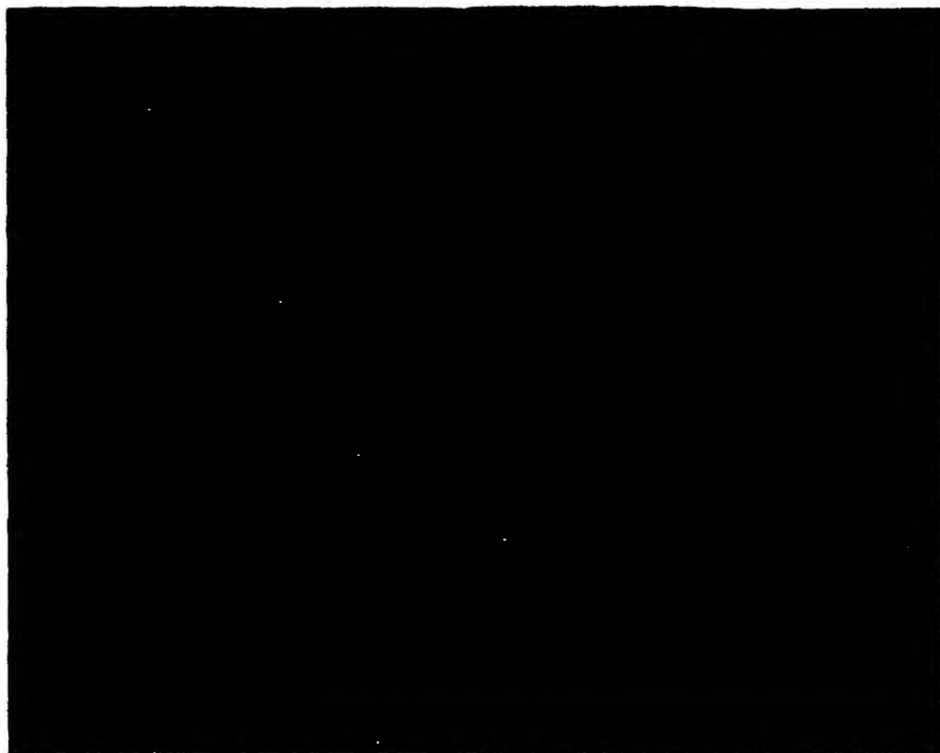

b

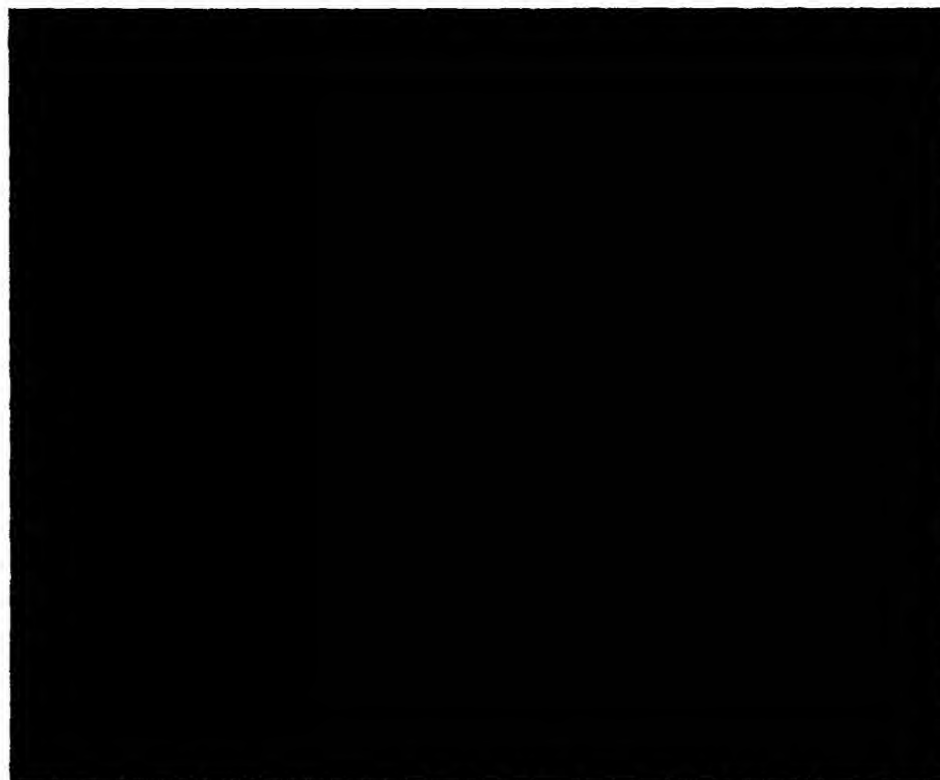


Fig. 5